



Model: GM1351

Digital Sound Level Meter Operation manual



Version: GM1351-EN-00

FGJ-NDT.IR

DIGINDT.IR

+982165565901

+982144584619

+989034119385

A. Introduction

This equipment has been designed to meet the measurement requirement of Safety Engineers, Health, Industrial Safety offices and Sound Quality control in various environment, which include factory, office, traffic, family, and audio system.

This equipment has the following functions:

1. It is designed according to the IEC651 TYPE2 & ANSI S1.4 TYPE2
2. Modern, compact, portable design
3. Accuracy up to ± 1.5 dB
4. Measurement range: 30dBA-130 dBA
5. MAX Hold
6. Auto backlight display
7. Auto power OFF

B. Safty Notice

Operation Environmental condition:

1. Below 2000 meters in height;
2. Humidity: <80%RH
3. Operation temperature: 0~40°C

Maintenance:

Use dry cloth to clean the unit, but never with any solvent.




Figure 1

C. Calibration Procedures

Please use a Standard Acoustic Calibrator.

1. Turn on the calibrator and set up the status to 94dB@1KHz.
2. Insert the microphone carefully into the 1/2 inch hole of the Calibrator.
3. Turn on the Calibrator and adjust the Protentiometer

inside the battery compartment of the unit (shown in the Figure 1), until the LCD display the desired Level 94.0dB.

**Our products are all well calibrated before Shipment.
Recommended recalibration cycle: 1 year.

D. Name and functions (Figure 2)

1. Electret Condenser Microphone.
2. LCD Display.
3. ON/OFF button
4. Maximum value hold button. (MAX)
5. Light sensor
6. Tripod mounting nut
7. Potentiometer
8. Windscreen





Figure 2


پتروفرهان گستر جنوب


E. LCD Display (Figure 3)

1. Low battery indication
2. Measuring Value
3. Maximum value icon
4. Measuring unit: dBA

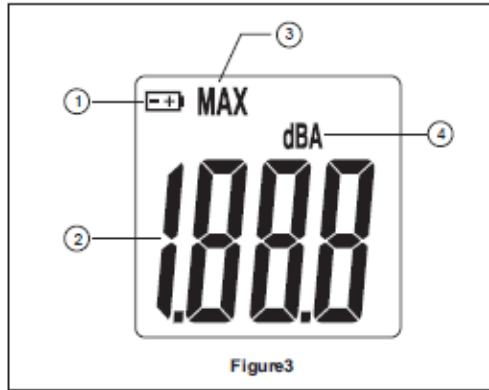



F. Pre-operations

1. Open the battery door and install 9V battery into the battery compartment.
2. Cover the battery door.
3. When Low battery mark "  " appears, please replaced with a new 9V battery. (Figure 4)



G. Operation

1. Standard measure mode
Press to "  " turn on the unit the LCD will display full screen for 1 second. Then it start to measure the current sound level.
The reading will changed according to the sound level of the current enviroment.
2. Max hold
Press "MAX" to lock the maximum sound level, the sound level will be locked until the higher value appears to replace. Press "MAX" again to go back the standard measure mode.
3. Auto backlight display
The light sensor will induct the light inteasity of enviroment automatically: when the light inteasity is insu-ficient, the backlight will be turned on automatically. It will changing according to the light inteasity.
4. Auto power off
This unit will shut off automatically in about 11 minutes.

To cancel this function, press "  " continuously till "UOF" display on the LCD, the auto power off function will be renewed in next turn on.

H. Caution

1. Do not operate the unit at high temperature and high humidity environment.
2. Please take out battery from unit if not in use for any extended period of time.
3. When using the unit in the presence of wind, mount the windsreen to avoid to pick up undesired signals.

I. Specification

Measuring range	30dBA-130dBA
Accuracy	± 1.5 dB (94dB@1KHz)
Frequency range	31.5Hz-8.5KHz
Frequency weighting	A
Digital Display	4digits
Resolution	0.1dB
Sample rate	2 times/second
Microphone	1/2 inch electret condenser microphone
Max Hold	MAX
Power supply	9V Battery
Power life	About 30 hours (alkaline battery)
Operating condition	0-40°C, 10-80%RH
Storage condition	-10-60°C, 10-70%RH
Weight	144g (including battery)
Dimension	57*26*149mm



MADE IN CHINA